

# ENALEES CENTRIEXTRACTION – BLOOD AND/OR URINE




Switch on and program the **instrument**.



Before opening the **tubes**, make sure that all the liquid and lyophilized pellets are at the bottom of the tubes.


1 ▶

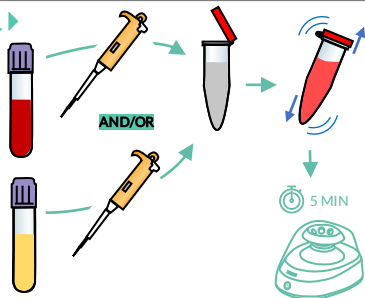

Collect a volume of blood, urine or one volume of each with the **orange pipette** fitted with a filter cone and transfer it to the **red tube**.


Shake vigorously the **red tube** and **centrifuge** it for at least 5 minutes.

2 ▶



Remove the supernatant of the **red tube** with **both sides** of the **saratige**.




3 ▶

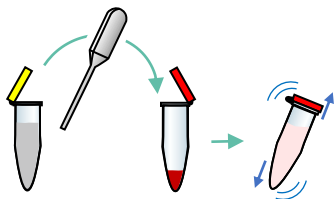

With the **albipette**, transfer the entire content of the **yellow tube** and dispense it in the **red tube**.

Shake vigorously the **red tube** to resuspend the cell pellet in the extraction buffer.

# ENALEES CENTRIEXTRACTION – BLOOD AND/OR URINE
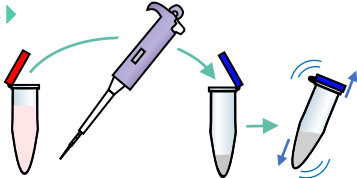
<p>4 ▶</p> 	<p>Draw liquid from the <b>red tube</b> with the <b>purple pipette</b> fitted with filter-tip.</p> <p>Transfer the liquid to the <b>blue tube</b> then shake it vigorously.</p>
<p>5 ▶</p> 	<p>Transfer liquid from the <b>blue tube</b> with the <b>orange pipette</b> fitted with filter-tip and dispense it in each minitube.</p>
<p>6 ▶</p> 	<p><b>Replace caps tightly</b> then shake the minitubes and make sure that all the droplets are at the bottom of the tubes.</p> <p>Insert the <b>minitubes</b> into the <b>instrument</b> (place the end tab on the left) then close immediately the lid of the <b>instrument</b> to start the analysis.</p>



Never reopen the minitubes once they have been inserted in the instrument, or after the end of the reaction.

Never leave the minitubes inside the instrument after the reaction has ended.

